Quick Start Guide

CORIS® Cleaning Cycle, Self-Disinfection Cycle, Adaptor Reprocessing

CORIS Accessories needed for the Endoscope Cleaning Cycle

CORIS Adaptor	Smart Drain Adaptor	Smart Seal
		

Cleaning Agent

CORIS QUANTUM® Cleaning Agent installed



CORIS QUANTUM Cleaning Agent

CORIS QUANTUM® Cleaning Agent must be installed before cleaning cycles can be run.

If the bottle is empty or no bottle is installed, press the notification on the Home screen and follow on-screen instructions to install a new bottle.



CORIS Endoscope Cleaning Cycle

To start an endoscope Cleaning Cycle:

1. Navigate to the Home Screen
2. Press the Start icon
3. Follow the on-screen instructions to complete the workflow



CORIS Accessories needed for Self-Disinfection

CORIS Bottle Plug	CORIS Adaptor Plug	CORIS SD Input Tube
		

Disinfectant


Revital-Ox RESERT HLD



CORIS Self-Disinfection

To start a Self-Disinfection Cycle:

1. Navigate to the Maintenance menu
2. Select CORIS Self-Disinfection Cycle
3. Follow the on-screen instructions to complete the workflow

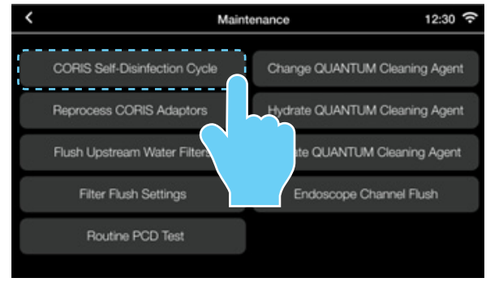

CORIS Accessories needed for Adaptor Reprocessing

CORIS Adaptor	Smart Drain Adaptor	CORIS Adaptor Reprocessing Hub	CORIS SD Input Tube
			

Disinfectant


Revital-Ox RESERT HLD



CORIS Adaptor Reprocessing

To start Adaptor Reprocessing:

1. Navigate to the Maintenance menu
2. Select Reprocess CORIS Adaptors
3. Follow the on-screen instructions to complete the workflow

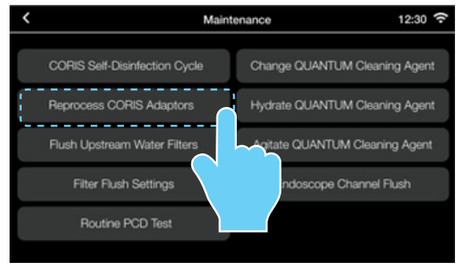

Consult the CORIS User Manual for instructions on operating the CORIS System.

© 2026 Nanosonics Limited. All rights reserved. 2352066-AU-UK-IRE-US-FLY-V01. June 2026