CORIS®

nanosonics
Infection Prevention. For Life.

Quick Reference Guide

CORIS Device and Accessory Maintenance

Maintenance Schedule

Daily
when in use

Exterior Wipe
- CORIS Device
- Smart Drain Port
- CORIS Adaptor
- Smart Drain Adaptor
- Adaptor Reprocessing Hub
- SD Input Tube
- Adaptor Plug
- Bottle Plug

Adaptor Reprocessing
- CORIS Adaptor
- Smart Drain Adaptor

Discard
- Smart Seal

Twice Weekly

Self-Disinfection
- CORIS Device

Consult the CORIS User Manual for detailed instructions on reprocessing the CORIS System

Daily

Discard Smart Seal

24h

The Smart Seal is 24 hour use only, discard after 24 hours.



Wipe the exterior of the Smart Seal as needed during use, in accordance with your facility's policies and procedures.


NOTE: Always consult the cleaning and disinfectant product's IFU for instructions and contact time.

NOTE: Always wear appropriate PPE when reprocessing any CORIS accessory.

Daily


Clean and Disinfect CORIS Adaptor and Smart Drain Adaptor



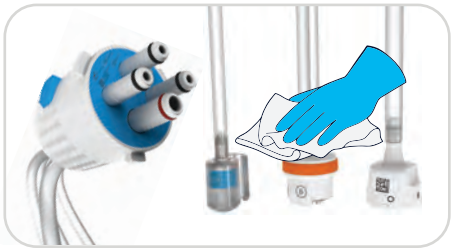

Clean and disinfect exterior surfaces of the CORIS Adaptor and Smart Drain Adaptor with a wipe, wait the full contact time.

Maintenance Options → Reprocess CORIS Adaptors

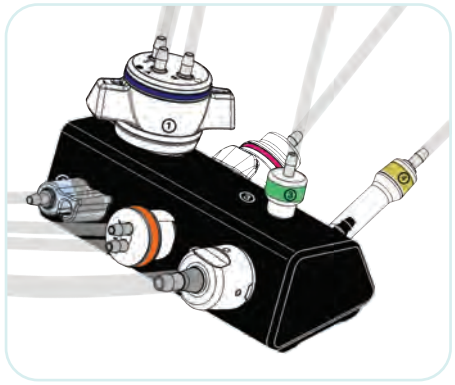

Reprocess the CORIS Adaptor and Smart Drain Adaptor using the Adaptor Reprocessing Hub.

Follow the on-screen instructions.

Refer to the **Revital-Ox® RESERT® HLD** IFU for correct usage. Connect the undiluted HLD to the CORIS Device via SD Input Tube.

After use in the Adaptor Reprocessing Cycle, clean and disinfect Adaptor Reprocessing Hub and SD Input Tube.



Clean and disinfect exterior surfaces of the Adaptor Reprocessing Hub and the SD Input Tube with a wipe, wait the full contact time.



Store the accessories in a clean, dry area.

Consult the CORIS User Manual for detailed instructions on reprocessing the CORIS System


CORIS®

Twice Weekly

Run the CORIS Self-Disinfection Cycle

Maintenance Options → CORIS Self-Disinfection Cycle

Self-Disinfect the CORIS Device using the Maintenance Kit. Follow the on-screen instructions.

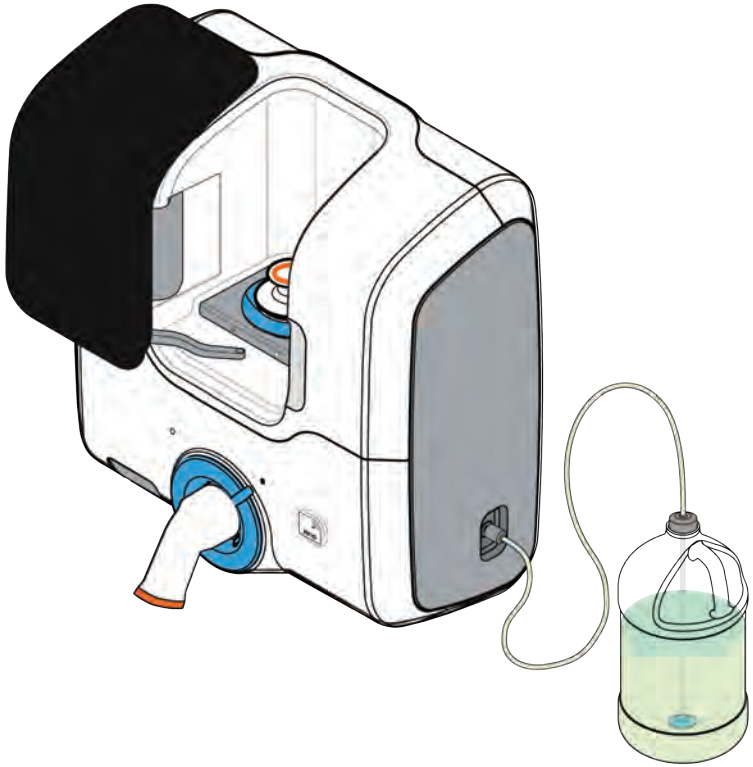

Refer to the **Revital-Ox® RESERT® HLD** IFU for correct usage. Connect the undiluted HLD to the CORIS Device via SD Input Tube.

After use in the Self-Disinfection Cycle, clean and disinfect the Maintenance Kit.



Clean and disinfect exterior surfaces of the Bottle Plug, Adaptor Plug and SD Input Tube with a wipe, wait the full contact time.



Store the Maintenance Kit in a clean, dry area.

Consult the CORIS User Manual for detailed instructions on reprocessing the CORIS System

CORIS®