CORIS®

nanosonics
Infection Prevention. For Life.

Quick Reference Guide

CORIS Device and Accessory Maintenance
with the Flushing Accessory

Maintenance Schedule

Daily
when in use

Exterior Wipe
- CORIS Device
- Smart Drain Port
- CORIS Adaptor
- Smart Drain Adaptor
- Flushing Accessory
- SD Input Tube
- Adaptor Plug
- Bottle Plug

Adaptor Reprocessing
- CORIS Adaptor
- Smart Drain Adaptor

Discard
- Smart Seal

Twice Weekly

Self-Disinfection
- CORIS Device

Consult the CORIS User Manual for detailed instructions on reprocessing the CORIS System

Daily

Discard Smart Seal

24h

The Smart Seal is 24 hour use only, discard after 24 hours.



Wipe the exterior of the Smart Seal as needed during use, in accordance with your facility's policies and procedures.


NOTE: Always consult the cleaning and disinfectant product's IFU for instructions and contact time.

NOTE: Always wear appropriate PPE when reprocessing any CORIS accessory.


Daily

Clean and Disinfect CORIS Adaptor and Smart Drain Adaptor with Flushing Accessory



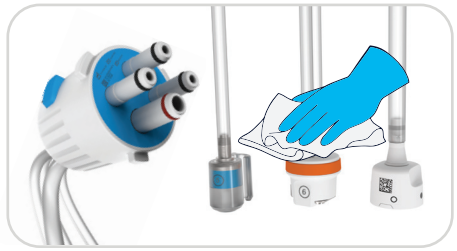


Clean and disinfect exterior surfaces of the CORIS Adaptor and Smart Drain Adaptor with a wipe. Leave visibly wet for required contact time.

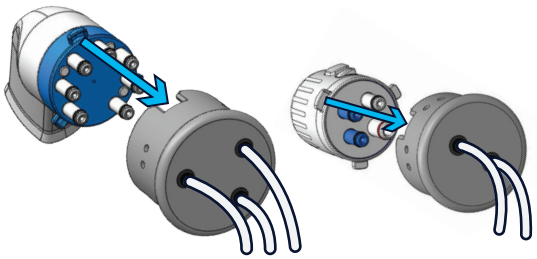


Connect the CORIS Adaptor to Adaptor Plate, press together fully.

Connect the Smart Drain Adaptor to Smart Drain Adaptor Plate, press together fully.

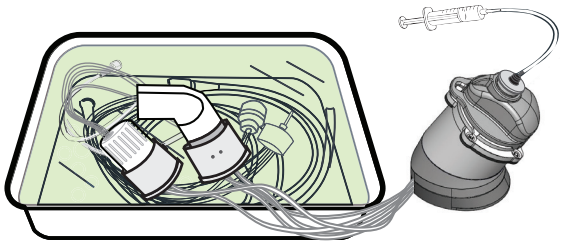


Place CORIS Adaptor, Smart Drain Adaptor, Flushing Accessory plates and inlet tube into clean basin.

Refer to the **Revital-Ox® RESERT® HLD** IFU for general instructions, then add undiluted disinfectant to fully submerge all the connectors and the inlet tube.

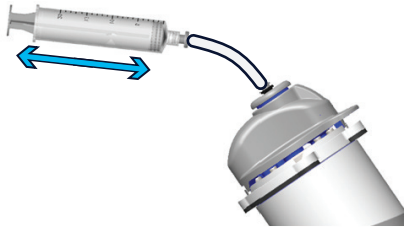

Start at position **A**.


Pump syringe **5** times.

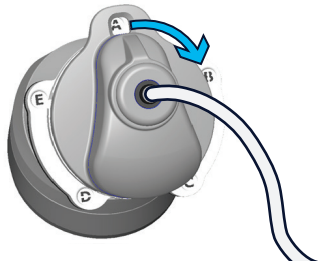

Rotate the dial clockwise to the next position.

Pump syringe **5** times.

Repeat for all positions: **A**, **B**, **C**, **D**, **E**.

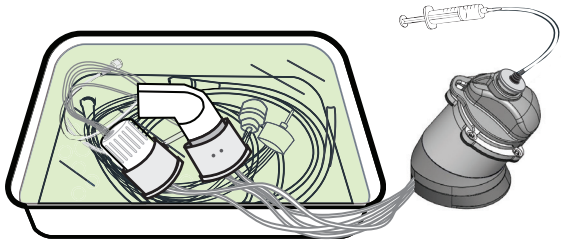


8 MINS

Wait the full 8 minute contact time.

Consult the CORIS User Manual for detailed instructions on reprocessing the CORIS System

Daily


Water Rinse of CORIS Adaptor and Smart Drain Adaptor

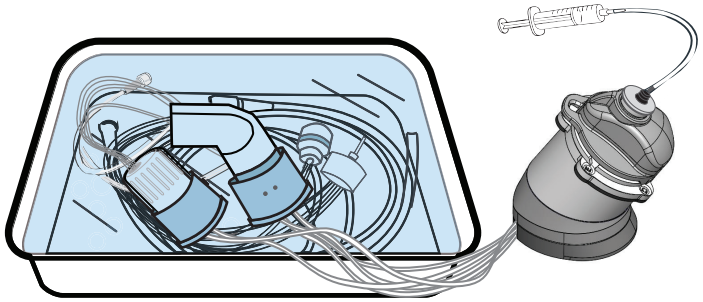

Fill a clean basin with potable water.

Transfer CORIS Adaptor, Smart Drain Adaptor, Flushing Accessory plates and inlet tube into water.

NOTE: Ensure all connectors and the inlet tube remain submerged.

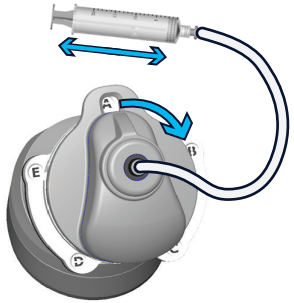


Start at position **A**.

Pump syringe **5** times.


Repeat for all positions:
A, **B**, **C**, **D**, **E**.

Air Purge of CORIS Adaptor and Smart Drain Adaptor

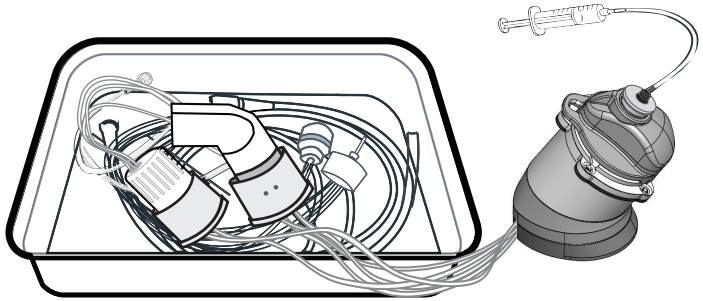

Transfer CORIS Adaptor, Smart Drain Adaptor, Flushing Accessory plates and inlet tube into a clean, dry basin.

NOTE: Ensure the inlet tube is positioned so it will remain free from liquid during air purge.

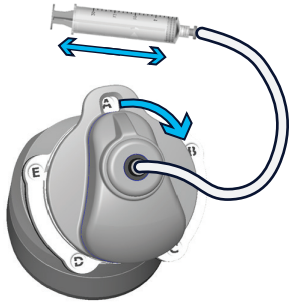

Start at position **A**.

Pump syringe **5** times.


Repeat for all positions:
A, **B**, **C**, **D**, **E**.

Consult the CORIS User Manual for detailed instructions on reprocessing the CORIS System

CORIS®

Daily

Drying and Storage of CORIS Adaptor and Smart Drain Adaptor

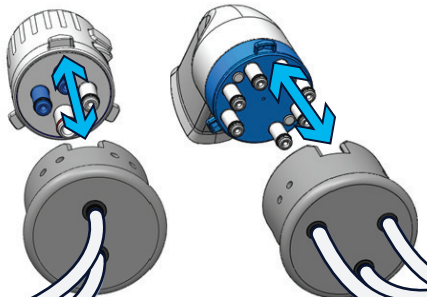

Place adaptors and Flushing Accessory on a clean, dry surface and disconnect.



Dry exterior surfaces of the adaptors using a sterile, low-lint, soft wipe.




Store adaptors by hanging them in a clean, dry area.

Cleaning and Disinfection of Flushing Accessory





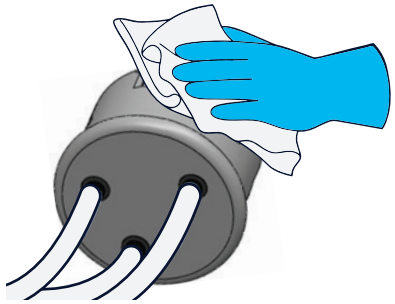

Clean and disinfect exterior surfaces of the Flushing Accessory with a wipe. Leave visibly wet for required contact time.

Store Flushing Accessory on a drying rack (or equivalent) in a clean, dry area.

Clean and disinfect exterior surfaces of the CORIS Adaptor and Smart Drain Adaptor with a wipe. Leave visibly wet for required contact time.

Consult the CORIS User Manual for detailed instructions on reprocessing the CORIS System


CORIS®

Twice Weekly

Run the CORIS Self-Disinfection Cycle

Maintenance Options → CORIS Self-Disinfection Cycle

Self-Disinfect the CORIS Device using the Maintenance Kit. Follow the on-screen instructions.

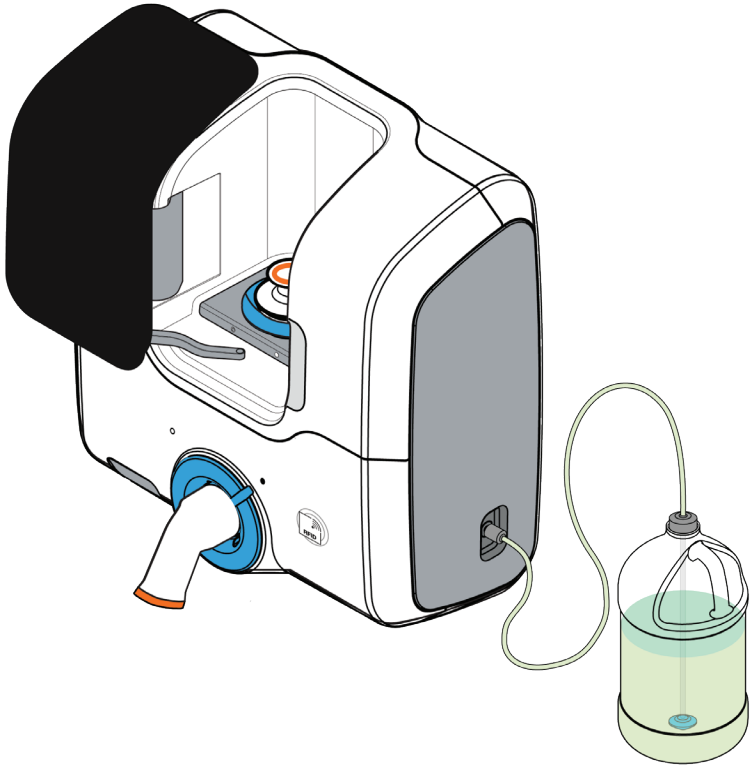

Refer to the **Revital-Ox® RESERT® HLD** IFU for general instructions. Connect the undiluted HLD to the CORIS Device via SD Input Tube.

After use in the Self-Disinfection Cycle, clean and disinfect the Maintenance Kit.



Clean and disinfect exterior surfaces of the Bottle Plug, Adaptor Plug and SD Input Tube with a wipe. Leave visibly wet for required contact time.



Store the Maintenance Kit in a clean, dry area.

Consult the CORIS User Manual for detailed instructions on reprocessing the CORIS System

CORIS®